


Quality control without Vis-NIR instrument



Quality control with Vis-NIR instrument

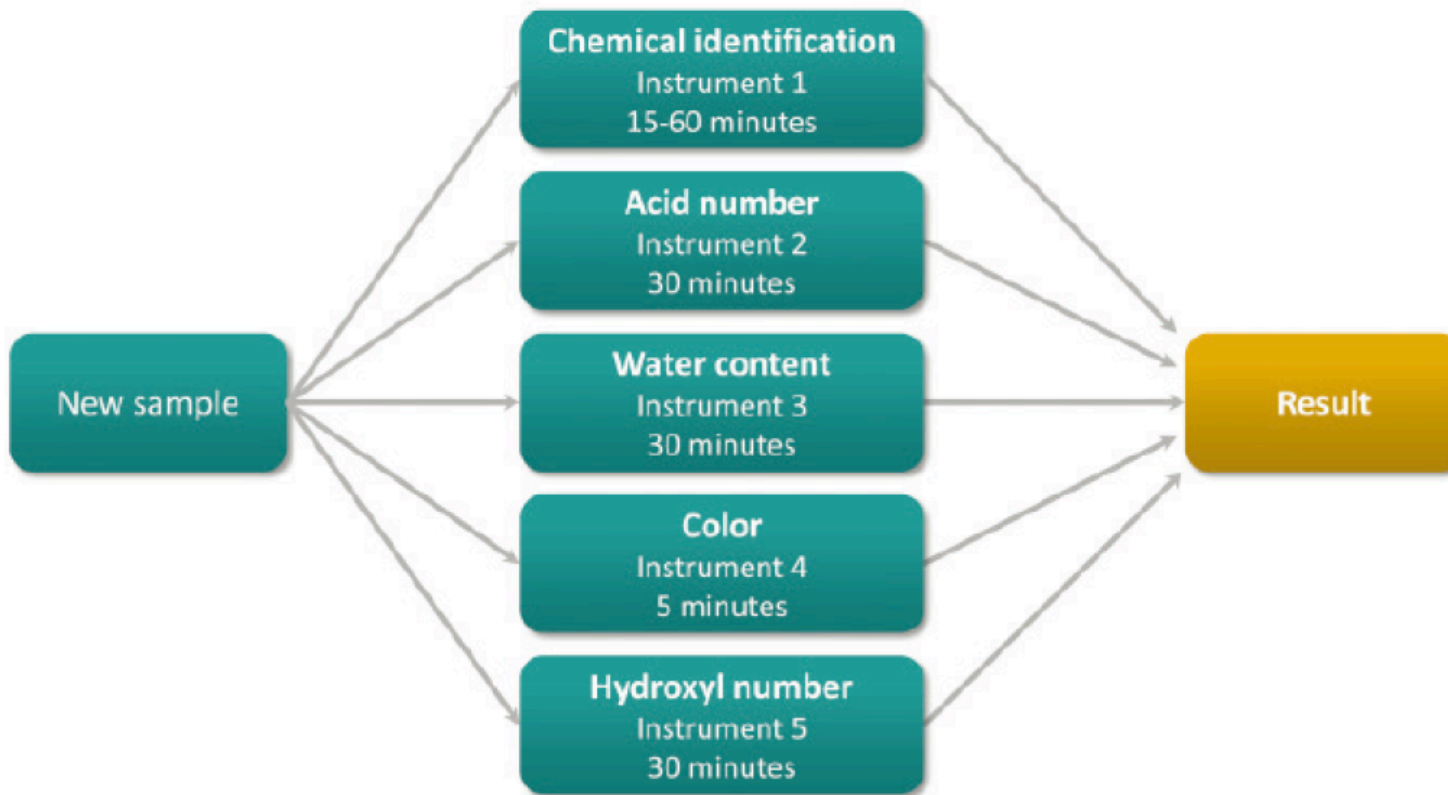